



Andrea Rockall
Andrew Hatrick
Peter Armstrong
Martin Wastie

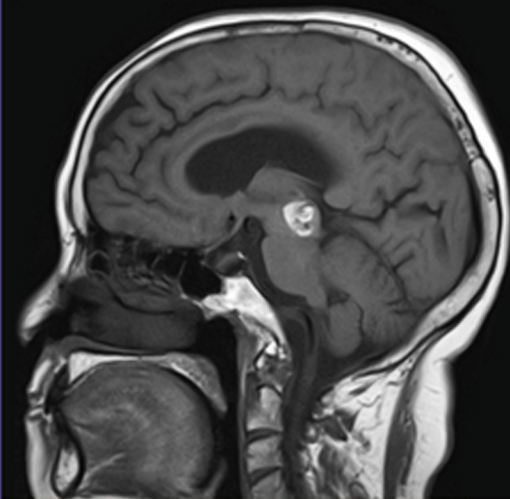

DIAGNOSTIC IMAGING

SEVENTH EDITION

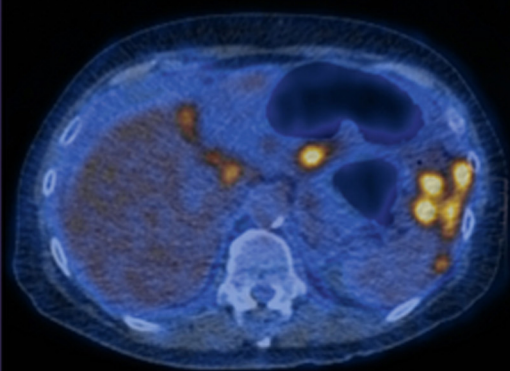


Wiley E-Text
Powered by VitalSource®

Available on
CourseSmart
Learn Smart. Choose Smart.



 **WILEY-BLACKWELL**

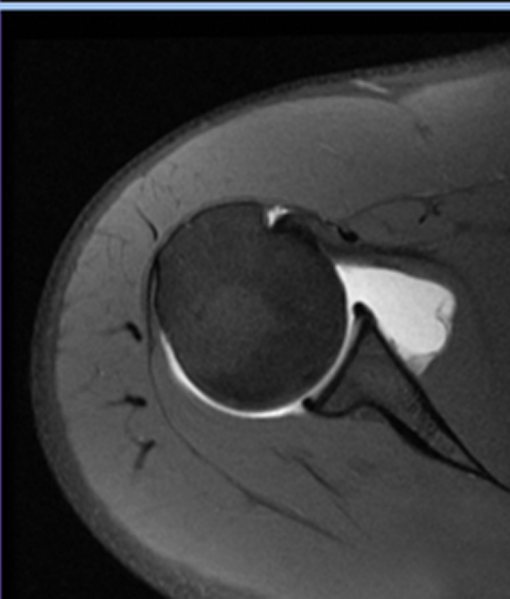

DIAGNOSTIC IMAGING

This new edition is also available as an e-book.

For more details, please see

www.wiley.com/buy/9780470658901

or scan this QR code:



Companion website

This book is accompanied by a companion website:

www.wileydiagnosticimaging.com

The website includes:

- Interactive multiple choice questions for each chapter
- Figures from the book in PowerPoint format

DIAGNOSTIC IMAGING

ANDREA ROCKALL

BSc, MBBS, MRCP, FRCR

Professor of Radiology

Imperial College, London, UK

ANDREW HATRICK

MA, MB BChir, MRCP, FRCR

Consultant General and Interventional Radiologist

Frimley Park Hospital NHS Foundation Trust

Frimley, UK

PETER ARMSTRONG

MBBS, FMed Sci, FRCP, FRCR

Formerly Professor of Radiology

Medical College of St Bartholomew's

and the Royal London Hospitals, London, UK

Formerly Professor and Vice-Chairman

Department of Radiology, University of Virginia

Charlottesville, Virginia, USA

MARTIN WASTIE

MB BChir, FRCP, FRCR

Formerly Professor of Radiology

University of Malaya Medical Centre

Kuala Lumpur, Malaysia

Formerly Consultant Radiologist

University Hospital, Nottingham, UK

SEVENTH EDITION

 **WILEY-BLACKWELL**

A John Wiley & Sons, Ltd., Publication

This edition first published 2013 © 2013 by A. Rockall, A. Hatrick, P. Armstrong, M. Wastie.
Previous editions published 1981 (as *X-ray Diagnosis*), 1987, 1992, 1998, 2004, 2009

Wiley-Blackwell is an imprint of John Wiley & Sons, formed by the merger of Wiley's global Scientific, Technical and Medical business with Blackwell Publishing.

Registered office: John Wiley & Sons, Ltd, The Atrium, Southern Gate, Chichester, West Sussex, PO19 8SQ, UK

Editorial offices: 9600 Garsington Road, Oxford, OX4 2DQ, UK
The Atrium, Southern Gate, Chichester, West Sussex, PO19 8SQ, UK
111 River Street, Hoboken, NJ 07030-5774, USA

For details of our global editorial offices, for customer services and for information about how to apply for permission to reuse the copyright material in this book please see our website at www.wiley.com/wiley-blackwell.

The right of the author to be identified as the author of this work has been asserted in accordance with the UK Copyright, Designs and Patents Act 1988.

All rights reserved. No part of this publication may be reproduced, stored in a retrieval system, or transmitted, in any form or by any means, electronic, mechanical, photocopying, recording or otherwise, except as permitted by the UK Copyright, Designs and Patents Act 1988, without the prior permission of the publisher.

Designations used by companies to distinguish their products are often claimed as trademarks. All brand names and product names used in this book are trade names, service marks, trademarks or registered trademarks of their respective owners. The publisher is not associated with any product or vendor mentioned in this book. This publication is designed to provide accurate and authoritative information in regard to the subject matter covered. It is sold on the understanding that the publisher is not engaged in rendering professional services. If professional advice or other expert assistance is required, the services of a competent professional should be sought.

Library of Congress Cataloging-in-Publication Data

Diagnostic imaging. — 7th ed. / Andrea G. Rockall ... [et al.].

p. ; cm.

Rev. ed. of: Diagnostic imaging / Peter Armstrong, Martin L. Wastie, Andrea G. Rockall. 6th ed. 2009.

Includes bibliographical references and index.

ISBN 978-0-470-65890-1 (pbk. : alk. paper)

I. Rockall, Andrea G. II. Armstrong, Peter, 1940– Diagnostic imaging.

[DNLM: 1. Diagnostic Imaging. WN 180]

616.07'54–dc23

201203

A catalogue record for this book is available from the British Library.

Wiley also publishes its books in a variety of electronic formats. Some content that appears in print may not be available in electronic books.

Cover image: © Andrea Rockall, Andrew Hatrick, Peter Armstrong, Martin Wastie
Cover design by Jim Smith

Set in 9/12 pt Palatino by Toppan Best-set Premedia Limited

Contents

- Preface, vii
- Acknowledgements, viii
- List of Abbreviations, ix
- The Anytime, Anywhere Textbook, x
- 1 Technical Considerations, 1
- 2 Chest, 19
- 3 Cardiac Disorders, 101
with the assistance of Dr Francesca Pugliese
- 4 Breast Imaging, 123
with the assistance of Dr Sarah Vinnicombe
- 5 Plain Abdomen, 129
- 6 Gastrointestinal Tract, 141
- 7 Hepatobiliary System, Spleen and Pancreas, 195
- 8 Urinary Tract, 223
- 9 Female Genital Tract, 273
- 10 Peritoneal Cavity and Retroperitoneum, 291
- 11 Bones, 309
with the assistance of Dr Kasthoori Jayarani
- 12 Joints, 347
with the assistance of Dr Kasthoori Jayarani
- 13 Spine, 369
with the assistance of Dr Rob Barker
- 14 Skeletal Trauma, 399
with the assistance of Dr Muaaze Ahmad
- 15 Brain, 427
with the assistance of Dr Rob Barker
- 16 Orbits, Head and Neck, 457
with the assistance of Dr Polly Richards
- 17 Vascular and Interventional Radiology, 471
- Appendix: Computed Tomography Anatomy of the Abdomen, 491
- Index, 497

Preface

Medical imaging is central to many aspects of patient management. Medical students and junior doctors can be forgiven their bewilderment when faced with the daunting array of information which goes under the heading 'Diagnostic imaging'. Plain film examinations remain the most frequently requested imaging investigations that non-radiologists may be called on to interpret and we continue to give them due emphasis. However, the use of cross-sectional imaging techniques continues to increase and, in some situations, has taken over from the plain film. The growing use of ultrasound, computed tomography (CT), magnetic resonance imaging (MRI), radionuclide imaging, including positron emission tomography (PET), and interventional radiology is reflected in the new edition.

With the widespread availability of most of the various imaging techniques, there are often several ways of investigating the same condition. We have avoided being too prescriptive as practice varies depending on the available equipment as well as the preferences of the clinicians and radiologists. It is important, however, to appreciate not

only the advantages but also the limitations of modern medical imaging.

We have continued to try to meet the needs of the medical student and doctors in training by explaining the techniques used in diagnostic imaging and the indications for their use. We aim to help the reader understand the principles of interpretation of imaging investigations. New for this edition is the availability of online material, including multiple choice questions for each chapter, allowing readers to test their knowledge.

It is beyond the scope of a small book such as this one to describe fully the pathology responsible for the various imaging appearances and the role of imaging in clinical management. Consequently, we encourage our readers to study this book in association with the study of these other subjects.

Andrea Rockall
Andrew Hatrick
Peter Armstrong
Martin Wastie

Acknowledgements

It would not have been possible to prepare this edition without the help of the many radiologists who have given ideas, valuable comments and inspiration. We would like to thank particularly the staff of the Radiology Departments at St Bartholomew's Hospital, London, Frimley Park NHS Trust, University Hospital, Nottingham, University of Malaya Medical Centre, Kuala Lumpur and County Hospital, Lincoln for this and past edition illustrations. Our special thanks go to those radiologists who gave us their expert assistance, including Dr Rob Barker, Dr Francesca Pugliese, Dr Sarah Vinnicombe, Dr Muaaze Ahmad, Dr Polly Richards and Dr Kasthoori Jayarani.

The following kindly provided illustrations for this and previous editions: Lorenzo Biassoni, Nishat Bharwani, John Bowe, Paul Clark, Siew Chen Chua, Peter Jackson, Jill Jacobs, Ranjit Kaur, Priya Narayanan, Steven Oscroft, Niall Power, Shaun Preston, Ian Rothwell, Peter Twining, Caroline Westerhout and Bob Wilcox.

We would like to thank Julie Jessop for her superb secretarial help and we would like to express our gratitude to the staff of Wiley-Blackwell.

List of Abbreviations

ADC	apparent diffusion coefficient	HMPAO	hexamethylpropyleneamine oxime
AIDS	acquired immune deficiency syndrome	HOCM	hypertrophic obstructive cardiomyopathy
ALARA	'as low as reasonably achievable' principle	HRCT	high resolution computed tomography
AP	anteroposterior	¹²³ I	iodine-123
ARDS	adult respiratory distress syndrome	¹³¹ I	iodine-131
AVM	arteriovenous malformation	IPF	idiopathic pulmonary fibrosis
BBB	blood–brain barrier	IUCD	intrauterine contraceptive device
CFA	cryptogenic fibrosing alveolitis	IVC	inferior vena cava
CPPD	calcium pyrophosphate dihydrate	IVU	intravenous urography
CSF	cerebrospinal fluid	^{81m} Kr	krypton-81m
CT KUB	non-contrast computed tomography of the kidneys, ureters and bladder	MAG-3	mercaptoacetyl triglycine
CT	computed tomography	MDCT	multidetector CT
CTR	cardiothoracic ratio	MEN	multiple endocrine neoplasia
CXR	chest radiograph	MIBG	meta-iodobenzylguanidine
3D	three-dimensional	MIP	maximum intensity projection
DCE-MRI	dynamic contrast-enhanced magnetic resonance imaging	MRA	magnetic resonance angiography
DEXA	dual-energy x-ray absorption	MRCP	magnetic resonance cholangiopancreatography
DMSA	dimercaptosuccinic acid	MRI	magnetic resonance imaging
DTPA	diethylene triamine pentacetic acid	NHS	National Health Service
DWI	diffusion-weighted imaging	PA	posteroanterior
ERCP	endoscopic retrograde cholangiopancreatography	PEG	percutaneous endoscopic gastrostomy
EUS	endoscopic ultrasound	PET	positron emission tomography
EVAR	endovascular aneurysm repair	PTC	percutaneous transhepatic cholangiogram
FAST	focused assessment with sonography for trauma	PUJ	pelviureteric junction
FDG	F-18 fluorodeoxyglucose	RIG	radiologically inserted gastrostomy
FDG-PET	fluorodeoxyglucose positron emission tomography	SCIWORA	spinal cord injury without radiological abnormality
FLAIR	fluid attenuated inversion recovery	SPECT	single photon emission computed tomography
FNA	fine needle aspiration	^{99m} Tc	technetium-99m
GI	gastrointestinal	TCC	transitional cell carcinoma
GIST	gastrointestinal stromal tumour	TIPSS	transjugular intrahepatic portosystemic shunt
HCC	hepatocellular carcinoma	TRUS	transrectal ultrasound
		UIP	interstitial pneumonia

The Anytime, Anywhere Textbook

Wiley E-Text Powered by VitalSource®

For the first time, your textbook comes with free access to a **Wiley E-Text: Powered by VitalSource** – a digital, interactive version of this textbook which you own as soon as you download it.

Your **Wiley E-Text: Powered by VitalSource** allows you to:

Search: Save time by finding terms and topics instantly in your book, your notes, even your whole library (once you've downloaded more textbooks)


Note and Highlight: Colour code, highlight and make digital notes right in the text so you can find them quickly and easily

Organize: Keep books, notes and class materials organized in folders inside the application

Share: Exchange notes and highlights with friends, classmates and study groups

Upgrade: Your textbook can be transferred when you need to change or upgrade computers

Link: Link directly from the page of your interactive textbook to all of the material contained on the companion website

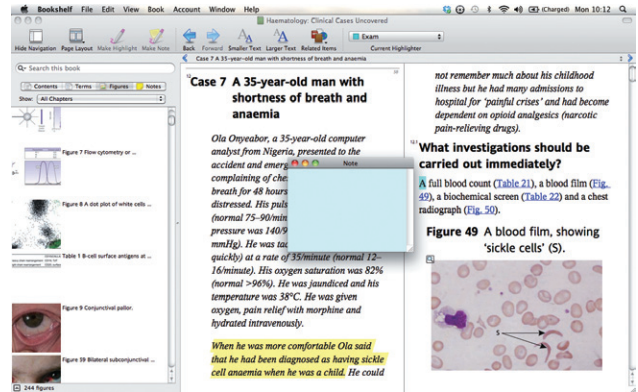

To access your Wiley E-Text: Powered by VitalSource:

- Find the redemption code on the inside front cover of this book and carefully scratch away the top coating of the label. Visit www.vitalsource.com/software/bookshelf/downloads to download the Bookshelf application to your computer, laptop or mobile device.
- If you have purchased this title as an e-book, access to your **Wiley E-Text: Powered by VitalSource** is available with proof of purchase within 90 days. Visit <http://support.wiley.com> to request a redemption code via the 'Live Chat' or 'Ask A Question' tabs.
- Open the Bookshelf application on your computer and register for an account.
- Follow the registration process and enter your redemption code to download your digital book.
- For full access instructions, visit www.wileydiagnosticimaging.com.

Available on
CourseSmart
Learn Smart. Choose Smart.



CourseSmart gives you instant access (via computer or mobile device) to this Wiley-Blackwell eTextbook and its extra electronic functionality, at 40% off the recommended retail print price. See all the benefits at www.coursesmart.com/students.

Instructors . . . receive your own digital desk copies!

It also offers instructors an immediate, efficient and environmentally-friendly way to review this textbook for your course.

For more information visit www.coursesmart.com/instructors.

With **CourseSmart**, you can create lecture notes quickly with copy and paste, and share pages and notes with your students. Access your Wiley **CourseSmart** digital textbook from your computer or mobile device instantly for evaluation, class preparation and as a teaching tool in the classroom.

Simply sign in at <http://instructors.coursesmart.com/bookshelf> to download your Bookshelf and get started. To request your desk copy, hit 'Request Online Copy' on your search results or book product page.

Companion website

This book is accompanied by a companion website:

www.wileydiagnosticimaging.com

The website includes:

- Interactive multiple choice questions for each chapter
- Figures from the book in PowerPoint format

Technical Considerations

Use of the imaging department

Good communication between clinicians and radiologists is vital because the radiology department needs to understand the clinical problem in order to carry out appropriate tests and to interpret the results in a meaningful way. Also, clinicians need to understand the strengths and limitations of the answers provided.

Sensible selection of imaging investigations is of great importance. There are two opposing philosophies. One approach is to request a battery of investigations, aimed in the direction of the patient's symptoms, in the hope that something will turn up. The other approach is 'trial and error': decide one or two likely diagnoses and carry out the appropriate test to support or refute these possibilities. We favour the selective approach as there is little doubt that the answers are usually obtained less expensively and with less distress to the patient. This approach depends on critical clinical evaluation; the more experienced the doctor, the more accurate he or she becomes in choosing appropriate tests.

Laying down precise guidelines for requesting imaging examinations is difficult because patients are managed differently in different centres. Box 1.1 provides important points when requesting imaging investigations.

Conventional radiography

X-rays are absorbed to a variable extent as they pass through the body. The visibility of both normal structures

Box 1.1 Best practice when requesting imaging investigations

- Only request an examination if it is likely to affect patient management
- The time interval between follow-up examinations should be appropriate and depends on the natural history of disease
- Localize the clinical problem as specifically as possible prior to imaging in order to reduce over-investigation and excess radiation exposure
- Careful consideration should be given to which imaging procedure is likely to give the relevant diagnostic information most easily
- Any investigations that have been requested but become unnecessary should be cancelled
- Examinations that minimize or avoid ionizing radiation should be chosen when possible
- Good communication with the radiologists is key to ensuring appropriate investigation pathways

and disease depends on this differential absorption. With conventional radiography there are four basic densities – gas, fat, all other soft tissues and calcified structures. X-rays that pass through air are least absorbed and, therefore, cause the most blackening of the radiograph, whereas calcium absorbs the most and so the bones and other calcified structures appear virtually white. The soft tissues, with the exception of fat, e.g. the solid viscera, muscle, blood, a variety of fluids, bowel wall, etc., all have similar absorptive capacity and appear the same shade of grey on conventional radiographs. Fat absorbs slightly fewer x-rays and, therefore, appears a little blacker than the other soft

tissues. Traditionally, images were produced using a silver-based photographic emulsion but now they are recorded digitally and viewed on computer screens in most centres.

Projections are usually described by the path of the x-ray beam. Thus, the term PA (posteroanterior) view designates that the beam passes from the back to the front, the standard projection for a routine chest film. An AP (anteroposterior) view is taken from the front. The term 'frontal' refers to either PA or AP projection. The image on an x-ray film is two-dimensional. All the structures along the path of the beam are projected on to the same portion of the film. Therefore, it is often necessary to take at least two views to gain information about the third dimension. These two views are usually at right angles to one another, e.g. the PA and lateral chest film. Sometimes two views at right angles are not appropriate and oblique views are substituted.

Portable x-ray machines can be used to take films of patients on the ward or in the operating theatre. Such machines have limitations on the exposures they can achieve. This usually means longer exposure times and poorer quality films. The positioning and radiation protection of patients in bed is often inferior to that which can be achieved within the x-ray department. Consequently, portable films should only be requested when the patient cannot be moved safely to the x-ray department.

Computed tomography

Computed tomography (CT) also relies on x-rays transmitted through the body. It differs from conventional radiography in that a more sensitive x-ray detection system is used, the images consist of sections (slices) through the body, and the data are manipulated by a computer. The x-ray tube and detectors rotate around the patient (Fig. 1.1). The outstanding feature of CT is that very small differences in x-ray absorption values can be visualized. Compared with conventional radiography, the range of densities recorded is increased approximately ten-fold. Not only can fat be distinguished from other soft tissues, but also gradations of density within soft tissues can be recognized, e.g. brain substance from cerebrospinal fluid, or tumour from surrounding normal tissues.

The patient lies with the body part to be examined within the gantry housing the x-ray tube and detectors. Although

other planes are sometimes practicable, axial sections are by far the most frequent. The operator selects the level and thickness to be imaged: the usual thickness is between 1.25 and 2 mm (often viewed by aggregating adjacent sections so they become 5 mm thick). The patient is moved past an array of detectors within the machine. In effect, the data at multiple adjacent levels are collected continuously, during which time the x-ray beam traces a spiral path to create a 'volume of data' within the computer memory. Multidetector (multislice) CT acquires multiple slices (64, 128, 256 or 320 depending on the machine) during one rotation of the x-ray tube. Multidetector CT enables the examination to be performed in a few seconds, thereby enabling hundreds of thin sections to be obtained in one breath-hold. A relatively new development is dual source (or dual energy) CT. This technique allows a virtual non-contrast CT image to be derived from CT acquired with intravenous iodinated contrast medium (see later in chapter) allowing a reduction in radiation dose in certain CT protocols.

The data obtained from the multislice CT exposures are reconstructed into an image by computer manipulation. The computer calculates the attenuation (absorption) value of each picture element (pixel). Each pixel is 0.25–0.6 mm in diameter, depending on the resolution of the machine, with a height corresponding to the chosen section thickness. The resulting images are displayed on a monitor and can be stored electronically. The attenuation values are expressed on an arbitrary scale (Hounsfield units) with water density being zero, air density being minus 1000 units and bone density being plus 1000 units (Fig. 1.2). The range and level of densities to be displayed can be selected by controls on the computer. The range of densities visualized on a particular image is known as the *window width* and the mean level as the *window level* or *window centre*. CT is usually performed in the axial plane, but because attenuation values for every pixel are present in the computer memory it is possible to reconstruct excellent images in other planes, e.g. coronal (Fig. 1.3), sagittal or oblique, and even three-dimensional (3D) images (Fig. 1.4).

The human eye can only appreciate a limited number of shades of grey. With a wide window all the structures are visible, but fine details of density difference cannot be appreciated. With a narrow window width, variations of just a few Hounsfield units can be seen, but much of the image is either totally black or totally white and in these

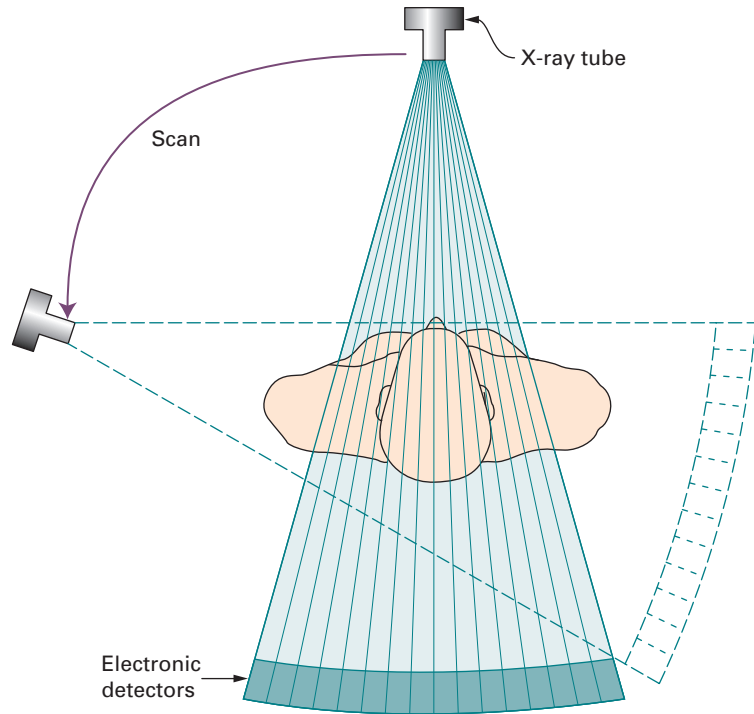


Fig. 1.1 Principle of CT. The x-ray tube and detectors move around the patient enabling a picture of x-ray absorption in different parts of the body to be built up.

areas no useful information is provided. The effects of varying window width and level are illustrated in Figs 1.5 and 2.6.

Computed tomography angiography

Rapid intravenous injections of contrast media result in significant opacification of blood vessels, which, with multiplanar or 3D reconstructions, can be exploited to produce angiograms. CT angiography, along with magnetic resonance angiography, is gradually replacing conventional diagnostic angiography.

Artefacts

There are numerous CT artefacts. The most frequent are those produced by movement and those from objects of very high density, such as barium in the bowel, metal

implants, dental fillings or surgical clips. Both types give rise to radiating linear streaks. The major problem is the resulting degradation of the image.

Contrast agents in conventional radiography and computed tomography

Radiographic contrast agents are used to visualize structures or disease processes that would otherwise be invisible or difficult to see. Barium is widely used to outline the gastrointestinal tract on conventional radiographic images; all the other radio-opaque media rely on iodine in solution to absorb x-rays. Iodine-containing solutions are used for urography, angiography and intravenous contrast enhancement at CT. Usually they are given in large doses, often with rapid rates of injection. As their only purpose is to produce opacification, ideally they should be pharmacologically inert. This has not yet been totally achieved,

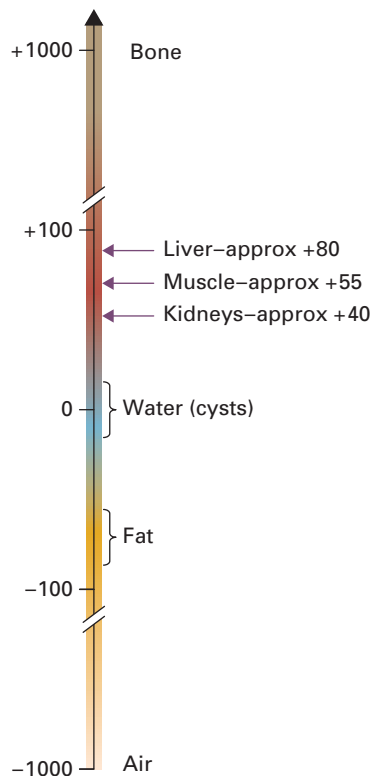


Fig. 1.2 Scale depicting the CT density (Hounsfield units) of various normal tissues in the body.

though the current low osmolality, non-ionic contrast media have exceedingly low complication rates.

Some patients experience a feeling of warmth spreading over the body as the iodinated contrast medium is injected. Contrast inadvertently injected outside the vein is painful and should be carefully guarded against. A few patients develop an urticarial rash, which usually subsides spontaneously.

Bronchospasm, laryngeal oedema or hypotension occasionally develop and may be so severe as to be life-threatening. It is therefore essential to be prepared for these dangerous reactions and to have available appropriate resuscitation equipment and drugs. Patients with known allergic manifestations, particularly asthma, are more likely to have an adverse reaction. Similarly, patients who have

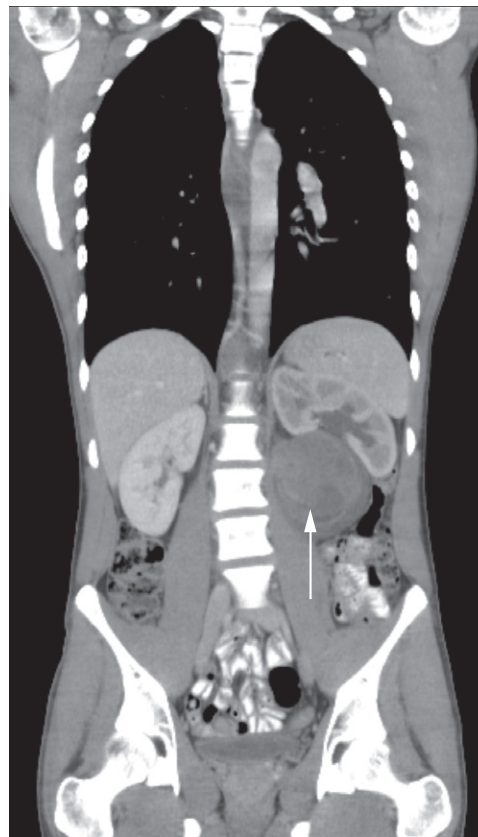


Fig. 1.3 Coronal reconstruction of CT of the chest, abdomen and pelvis. The images were obtained in the axial plane using very thin sections and then reconstructed into the desired plane – a coronal plane in this example. The illustrated section is through the posterior abdomen and shows the kidneys. There is a retroperitoneal mass (arrow) displacing the left kidney and causing hydronephrosis.

had a previous reaction to contrast agents have a higher than average risk of problems during the examination and an alternative method of imaging should be considered. Patients at higher risk are observed following the procedure. Intravenous contrast agents may have a deleterious effect on renal function in patients with impaired kidneys. Therefore, their use should be considered carefully on an individual basis and the patient should be well hydrated prior to injection.

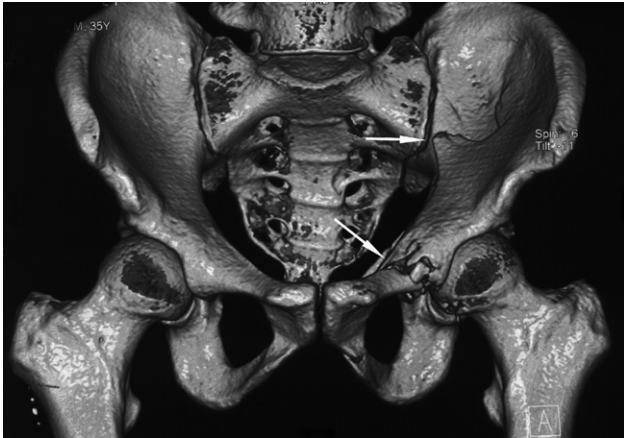


Fig. 1.4 Shaded surface 3D CT reconstruction. The images can be viewed in any desired projection and give a better appreciation of the pelvis. Two fractures are demonstrated in the left innominate bone (arrows), which were hard to diagnose on plain film.


Ultrasound

In diagnostic ultrasound examinations, very high frequency sound is directed into the body from a transducer placed in contact with the skin. In order to make good acoustic contact, the skin is smeared with a jelly-like substance. As the sound travels through the body, it is reflected by the tissue interfaces to produce echoes which are picked up by the same transducer and converted into an electrical signal.


As air, bone and other heavily calcified materials absorb nearly all the ultrasound beam, ultrasound plays little part in the diagnosis of lung or bone disease. The information from abdominal examinations may be significantly impaired by gas in the bowel, which interferes with the transmission of sound.

Fluid is a good conductor of sound, and ultrasound is, therefore, a particularly good imaging modality for diagnosing cysts, examining fluid-filled structures such as the bladder and biliary system, and demonstrating the fetus in its amniotic sac. Ultrasound can also be used to demonstrate solid structures that have a different acoustic impedance to adjacent normal tissues, e.g. metastases.

Ultrasound is often used to determine whether a structure is solid or cystic (Fig. 1.6). Cysts or other fluid-filled

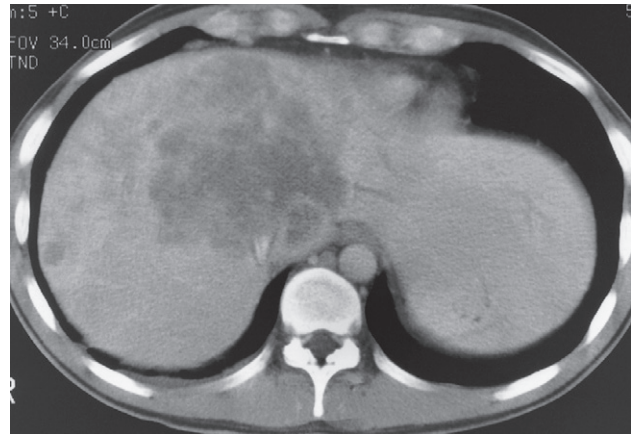

(a)

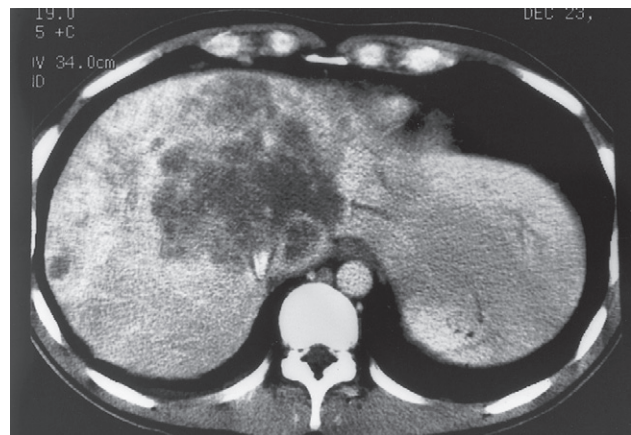

(b)

Fig. 1.5 Effect of varying window width on CT. In (a) and (b) the level has been kept constant at 65 Hounsfield units (HU). The window width in (a) is 500HU whereas in (b) it is only 150HU. Note that in the narrow window image (b), the metastases are better seen, but that structures other than the liver are better seen in (a).

structures produce echoes from their walls but no echoes from the fluid contained within them. Also, more echoes than usual are received from the tissues behind the cyst, an effect known as *acoustic enhancement*. Conversely, with a calcified structure, e.g. a gall stone (Fig. 1.7), there is a great reduction in the sound that will pass through, so a band of

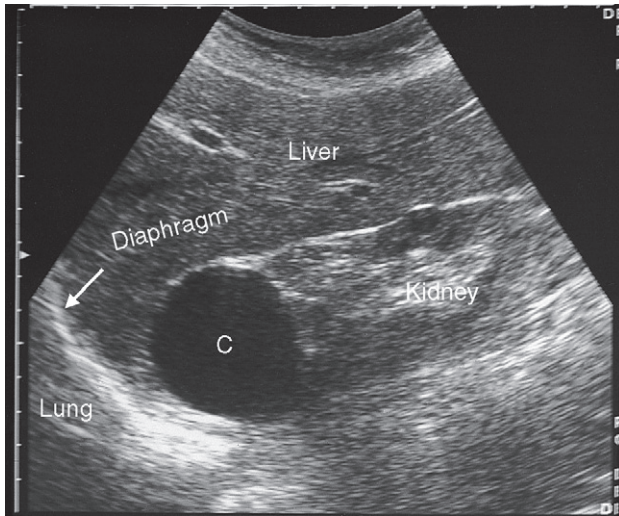


Fig. 1.6 Ultrasound scan of longitudinal section through the liver and right kidney. A cyst (C) is present in the upper pole of the kidney.

reduced echoes, referred to as an *acoustic shadow*, is seen behind the stone.

Ultrasound is produced by causing a special crystal to oscillate at a predetermined frequency. Very short pulses of sound lasting about a millionth of a second are transmitted approximately 500 times each second. The crystal not only transmits the pulses of sound but also 'listens' to the returning echoes, which are electronically amplified to be recorded as signals on a television monitor. Photographic or video reproductions of the image can provide a permanent record.

The time taken for each echo to return to the transducer is proportional to the distance travelled. Knowledge of the depth of the interface responsible for the echoes allows an image to be produced. Also, by knowing the velocity of sound in tissues, it is possible to measure the distance between interfaces. This is of great practical importance in obstetrics, for example, where the measurement of fetal anatomy has become the standard method of estimating fetal age.

During the scan, the ultrasound beam is electronically swept through the patient's body and a section of the internal anatomy is instantaneously displayed. The resulting image is a slice, so in order to obtain a 3D assessment a

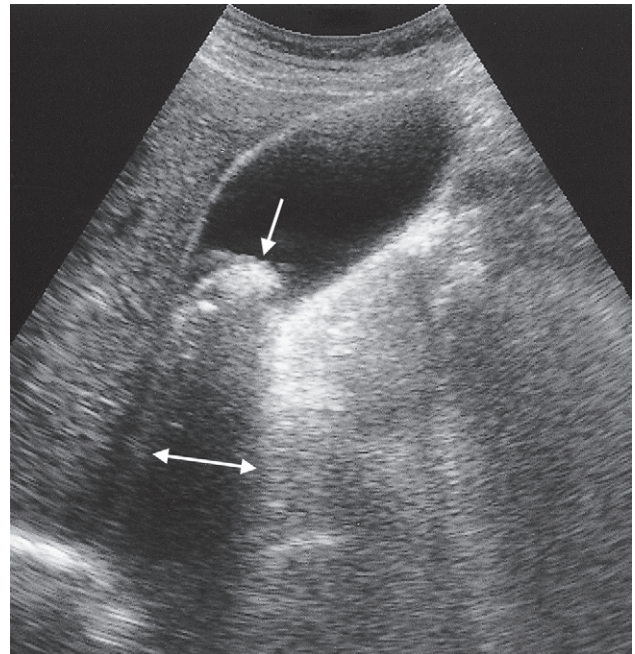


Fig. 1.7 Ultrasound scan of gall bladder showing a large stone in the neck of the gall bladder (downward pointing arrow). Note the acoustic shadow behind the stone (horizontal double-headed arrow).

number of slices must be created by moving or angling the transducer.

Unlike other imaging modalities, there are no fixed projections and the production of the images and their subsequent interpretation depend very much on the observations of the operator during the examination. Ultrasound images are capable of providing highly detailed information, e.g. very small lesions can be demonstrated (Fig. 1.8).

Small ultrasound probes, which may be placed very close to the region of interest, produce highly detailed images but with a limited range of a few centimetres. Examples are rectal probes for examining the prostate and transvaginal probes for the examination of the pelvic structures. Tiny ultrasound probes may be incorporated in the end of an endoscope. Lesions of the oesophagus, heart and aorta may be demonstrated with an endoscope placed in the oesophagus, and lesions of the pancreas may be detected with an endoscope passed into the stomach and duode-

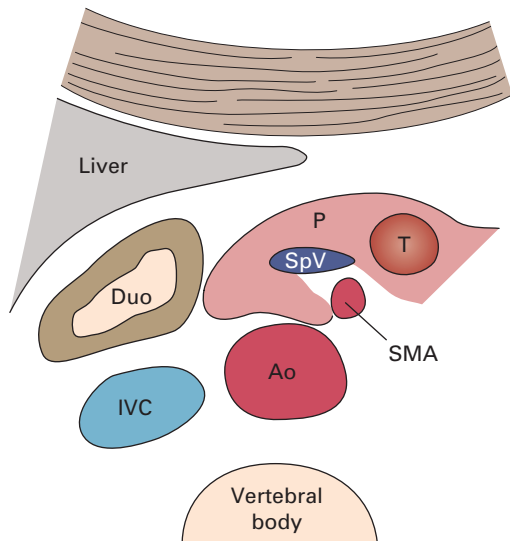
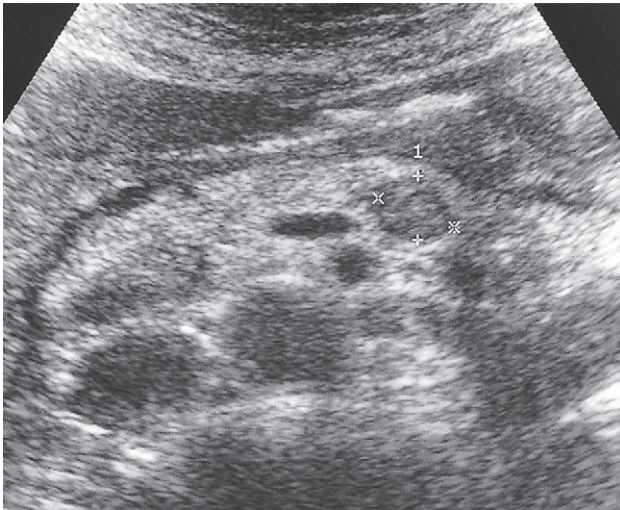


Fig. 1.8 Ultrasound scan of pancreas showing a 1 cm tumour (T) (an insulinoma) at the junction of the head and body of the pancreas. Ao, aorta; Duo, duodenum; IVC, inferior vena cava; P, pancreas; SMA, superior mesenteric artery; SpV, splenic vein.

num. Special ultrasound probes have also been developed that can be inserted into arteries to detect atheromatous disease.

Three-dimensional ultrasound has been recently developed and is used primarily in obstetrics to obtain 3D

images of the fetus. A conventional ultrasound transducer is used, which is moved slowly across the body recording simultaneously the location and ultrasound image. A 3D image can be constructed from the data received.

At the energies and doses currently used in diagnostic ultrasound, no harmful effects on any tissues have been demonstrated.

Ultrasound contrast agents have been developed. These agents contain microscopic air bubbles that enhance the echoes received by the probe. The air bubbles are held in a stabilized form, so they persist for the duration of the examination, and blood flow and perfusion to organs can be demonstrated. The technique is used to help characterize liver and renal abnormalities and in the investigation of cardiac disease.

Doppler effect

Sound reflected from a mobile structure shows a variation in frequency that corresponds to the speed of movement of the structure. This shift in frequency, which can be converted to an audible signal, is the principle underlying the Doppler probe used in obstetrics to listen to the fetal heart.

The Doppler effect can be exploited to image blood flowing through the heart or blood vessels. Here the sound is reflected from the blood cells flowing in the vessels (Fig. 1.9). If blood is flowing towards the transducer, the received signal is of higher frequency than the transmitted frequency, whilst the opposite pertains if blood is flowing away from the transducer. The difference in frequency between the sound transmitted and received is known as the Doppler frequency shift (Box 1.2). The direction of blood flow can readily be determined and flow towards the transducer is, by convention, coloured red, whereas blue indicates flow away from the transducer.

When a patient is being scanned, the Doppler information in colour is superimposed onto a standard ultrasound image (Fig. 1.10).

During the examination, the flow velocity waveform can be displayed and recorded. As the waveforms from specific arteries and veins have characteristic shapes, flow abnormalities can be detected. If the Doppler angle (Fig. 1.9) is known then the velocity of the flowing blood can be calculated, and blood flow can be calculated provided the diameter of the vessel is also known.

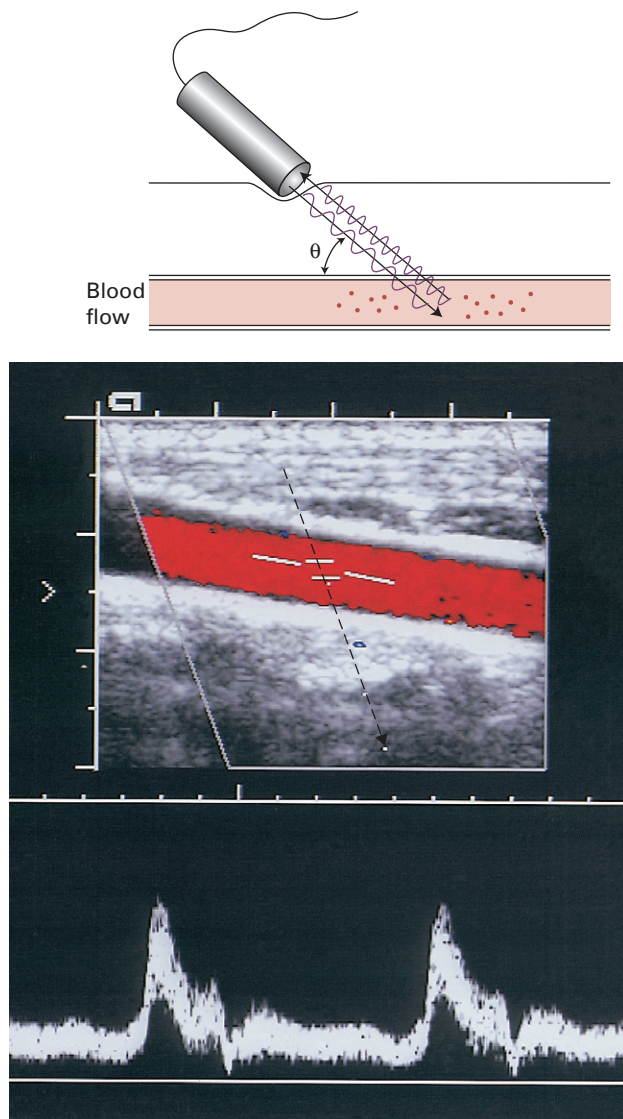


Fig. 1.9 Principle of Doppler ultrasound. In this example, flowing blood is detected in a normal carotid artery in the neck. With blood flowing away from the transducer, the frequency of the received sound is reduced, whereas with blood flowing towards the transducer, the frequency of the received sound is increased. For anatomical images, the flowing blood is colour coded according to the direction of flow. (θ is the angle between the vessel and the transmitted sound wave: an angle known as the Doppler angle. The angle of the beam is indicated by the fine zig-zag line across the image.) The flow-velocity waveform has been taken from the gate within the artery. The peaks represent systolic blood flow.

Box 1.2 Doppler frequency shift formula

$$\text{Frequency shift} = \frac{2Fi \times V \times \cos \theta}{c}$$


As c , the speed of sound in tissues, and Fi , the incident frequency of sound, are constant, and if θ , the Doppler angle, is kept constant, the frequency shift depends directly on the blood flow velocity V

Doppler studies are used to detect venous thrombosis, arterial stenosis and occlusion, particularly in the carotid arteries. In the abdomen, Doppler techniques can determine whether a structure is a blood vessel and can help in assessing tumour blood flow. In obstetrics, Doppler ultrasound is used particularly to determine fetal blood flow through the umbilical artery. With Doppler echocardiography it is possible to demonstrate regurgitation through incompetent valves and pressure gradients across valves can be calculated.


Radionuclide imaging

The radioactive isotopes used in diagnostic imaging emit gamma-rays as they decay. Gamma-rays are electromagnetic radiation, similar to x-rays, produced by radioactive decay of the nucleus. Many naturally occurring radioactive isotopes, e.g. potassium-40 and uranium-235, have half lives of hundreds of years and are, therefore, unsuitable for diagnostic imaging. The radioisotopes used in medical diagnosis are artificially produced and most have short half lives, usually a few hours or days. To keep the radiation dose to the patient at a minimum, the smallest possible dose of an isotope with a short half life should be used. Clearly, the radiopharmaceuticals should have no undesirable biological effects and should be rapidly excreted from the body following completion of the investigation.


Radionuclides can be chemically tagged to certain substances that concentrate selectively in different parts of the body. Occasionally, the radionuclide in its ionic form will selectively concentrate in an organ, so there is no need to attach it to another compound. Such a radionuclide is technetium-99m (^{99m}Tc). It is readily prepared, has a convenient half life of 6 hours and emits gamma-radiation of a suitable energy for easy detection. Other radionuclides that are used include indium-111, gallium-67, iodine-123 and thallium-201.

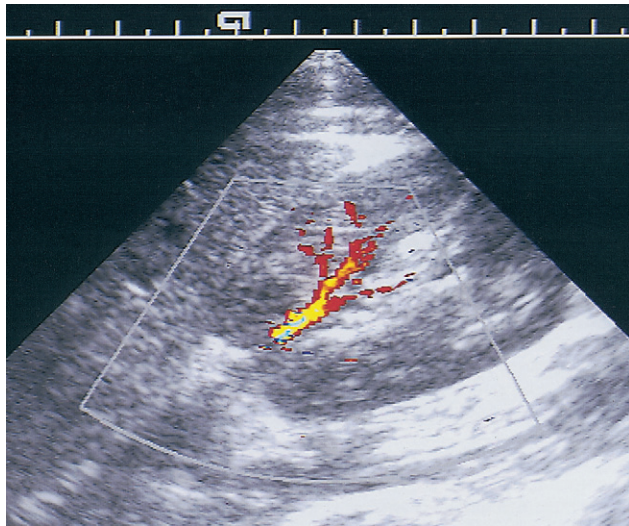

(a)

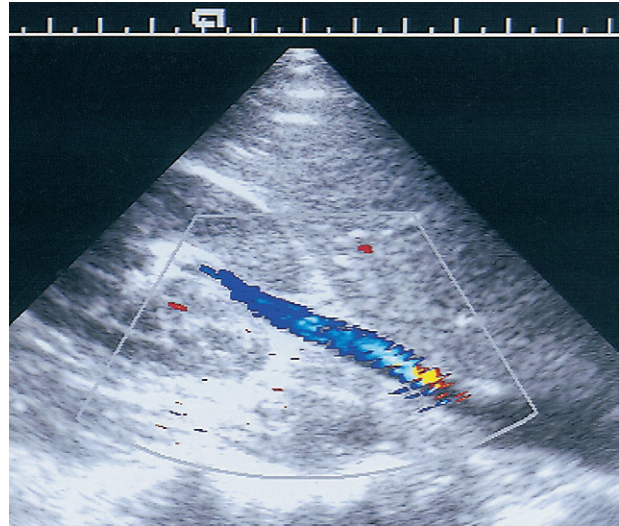

(b)

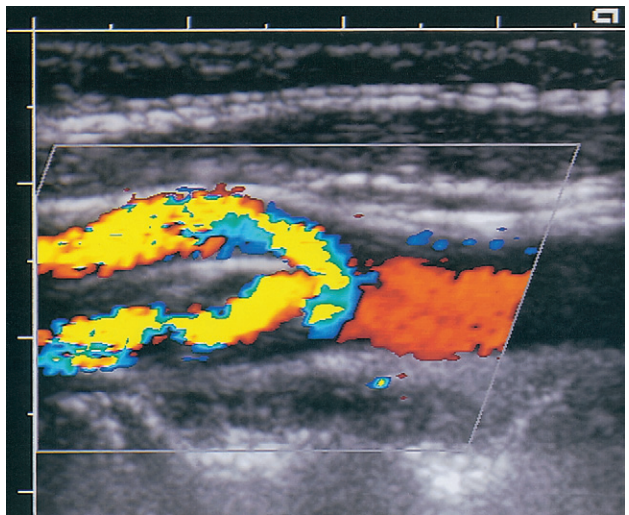

(c)

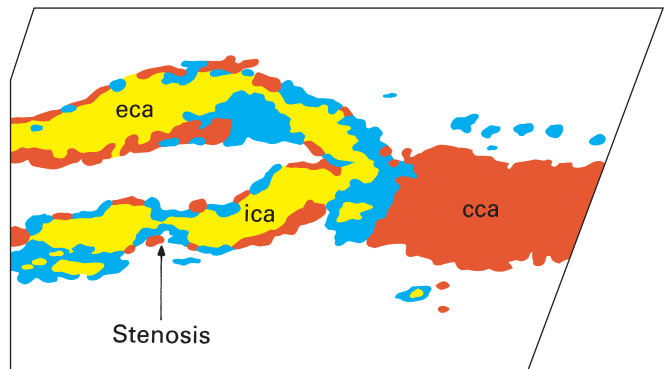


Fig. 1.10 Colour Doppler. (a) Normal renal artery. (b) Normal renal vein. (c) Bifurcation of the common carotid artery showing stenosis of the internal carotid artery. The flowing blood is revealed by colour. The precise colour depends on the speed and direction of the blood flow. cca, common carotid artery; eca, external carotid artery; ica, internal carotid artery.

Technetium-99m can be used in ionic form (as the pertechnetate) to detect ectopic gastric mucosa in Meckel's diverticulum, but it is usually tagged to other substances. For example, a complex organic phosphate labelled with ^{99m}Tc will be taken up by the bones and can be used to visu-

alize the skeleton (Fig. 1.11). Particles are used in lung perfusion images; macroaggregates of albumin with a particle size of 10–75 μm when injected intravenously are trapped in the pulmonary capillaries. If the macroaggregates are labelled with ^{99m}Tc , then the blood flow to the

lungs can be visualized. It is also possible to label the patient's own red blood cells with ^{99m}Tc to assess cardiac function, or the white cells with indium-111 or ^{99m}Tc for abscess detection. Small quantities of radioactive gases, such as xenon-133, xenon-127 or krypton-81m, can be inhaled to assess ventilation of the lungs. All these radiopharmaceuticals are free of side-effects.

The gamma-rays emitted by the isotope are detected by a gamma camera, enabling an image to be produced. A gamma camera consists of a large sodium iodide crystal, usually 40cm in diameter, coupled to a number of photomultiplier tubes. Light is produced when the gamma-rays strike and activate the sodium iodide crystal, and the light is then electronically amplified and converted to an electri-

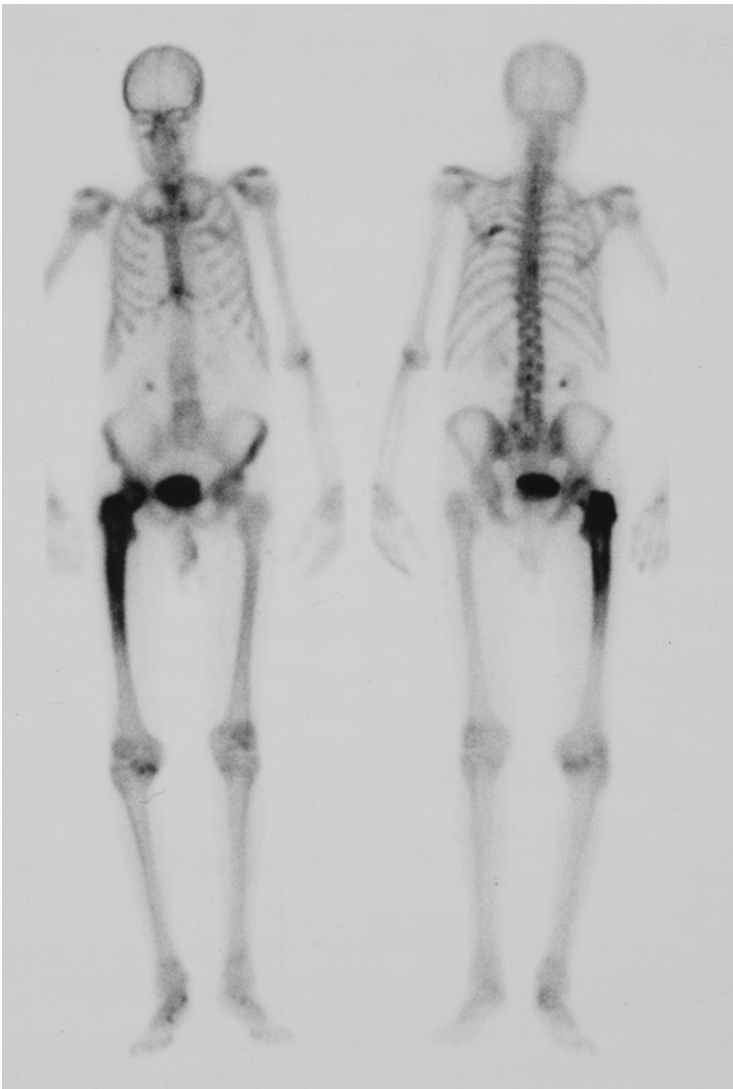


Fig. 1.11 Radionuclide bone scan. The patient has received an intravenous injection of a ^{99m}Tc -labelled bone-scanning agent (a complex organic phosphate). This agent is taken up by bone in proportion to bone turnover and blood flow. The increased uptake in the femur in this patient was due to Paget's disease.

cal pulse. The electrical pulse is further amplified and analyzed by a processing unit so that a recording can be made. Invariably, some form of computer is linked to the gamma camera to enable rapid serial images to be taken and to perform computer enhancement of the images when relevant.

In selected cases emission tomography is performed. In this technique, the gamma camera moves around the patient. A computer can analyze the information and produce sectional images similar to CT. Emission tomography can detect lesions not visible on the standard views. Because only one usable photon for each disintegration is emitted, this technique is also known as single photon emission computed tomography (SPECT).

Nuclear medicine techniques are used to measure function and to produce anatomical images. Even the anatomical images are dependent on function; for example, a bone scan depends on bone turnover. The anatomical informa-

tion they provide, however, is limited by the relatively poor spatial resolution of the gamma camera compared with other imaging modalities.

Positron emission tomography

Positron emission tomography (PET) uses short-lived positron-emitting isotopes, which are produced by a cyclotron immediately before use. Two gamma-rays are produced from the annihilation of each positron and can be detected by a specialized gamma camera. The resulting images reflect the distribution of the isotope (Fig. 1.12a). By using isotopes of biologically important elements such as carbon or oxygen, PET can be used to study physiological processes such as blood perfusion of tissues, and metabolism of substances such as glucose, as well as complex biochemical pathways such as neurotransmitter storage and binding. The most commonly used agent is

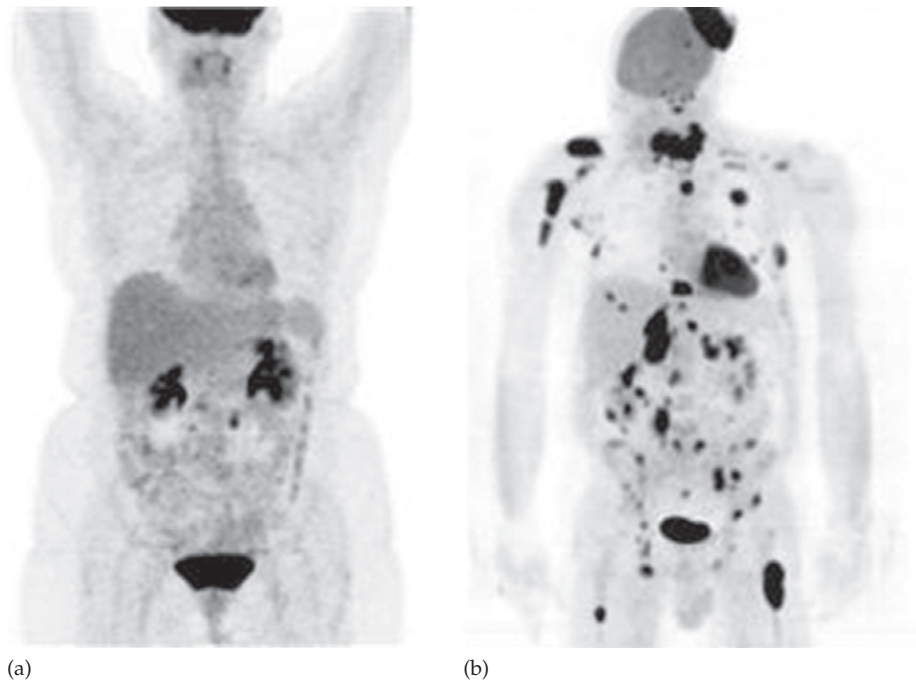


Fig. 1.12 FDG-PET scans, maximum intensity projections. (a) Normal isotope distribution. There is intense uptake in the brain and the neck uptake is in the tonsils. The FDG is excreted by the kidneys. (b) Lymphoma, showing multiple visceral, nodal, bone and scalp deposits.

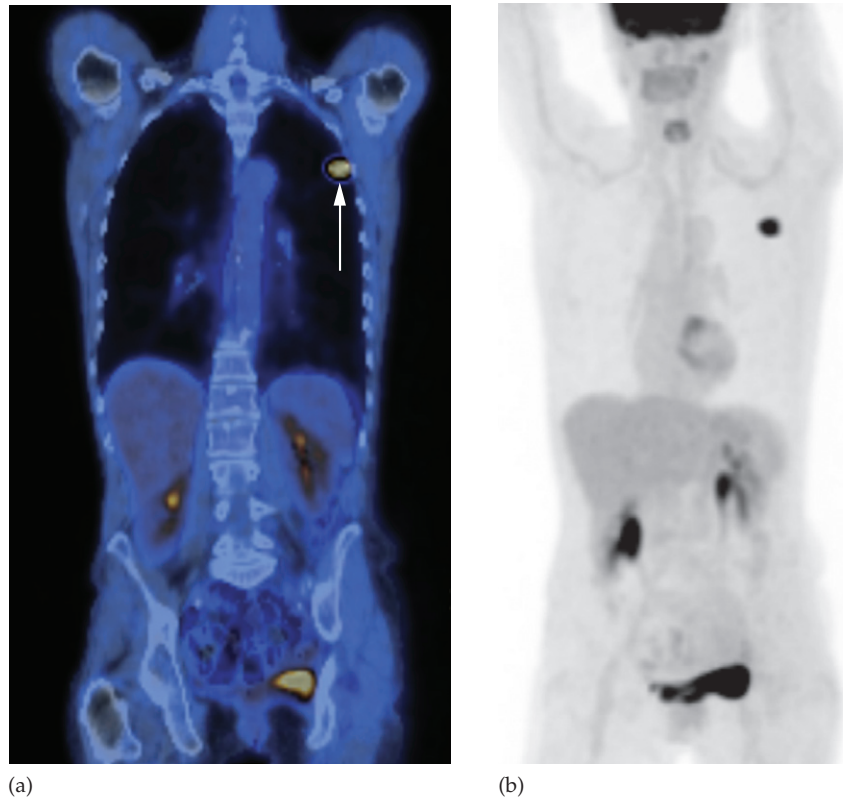


Fig. 1.13 FDG-PET/CT of lung cancer. (a) Coronal fused image and (b) maximum intensity projection, demonstrating a small left lung cancer (arrowed in (a)). The remainder of the FDG uptake is physiological.

F-18 fluorodeoxyglucose (FDG). This is an analogue of glucose and is taken up by cells in proportion to glucose metabolism, which is usually increased in tumour cells. Because muscle activity results in the uptake of FDG, the patient should rest quietly in the interval between injection of the FDG and scanning.

The images must be interpreted carefully as non-cancerous conditions may show uptake resembling cancer. PET using FDG is the most sensitive technique for staging solid tumours, such as bronchial carcinoma (Fig. 1.13), and in the follow-up of malignancies, particularly lymphoma (Fig. 1.12b), where other imaging techniques may be unable to distinguish active disease from residual fibrosis.

Positron emission tomography is also used in the evaluation of ischaemic heart disease and in brain disorders such as dementia, epilepsy and Parkinson's disease.

Positron emission tomography demonstrates biological function while CT gives anatomical information. If PET and CT are fused, the lesions detected by PET can be precisely localized by CT (Fig. 1.13). Modern equipment allows both PET and CT to be performed sequentially on the same machine.

Magnetic resonance imaging

The basic principles of magnetic resonance imaging (MRI) depend on the fact that the nuclei of certain elements align with the magnetic force when placed in a strong magnetic field. At the field strengths currently used in medical imaging, hydrogen nuclei (protons) in water molecules and lipids are responsible for producing anatomical images. If a radiofrequency pulse at the resonant frequency of hydro-

gen is applied, a proportion of the protons change alignment, flipping through a preset angle, and rotate in phase with one another. Following this radiofrequency pulse, the protons return (realign) to their original positions. As the protons realign (relax), they induce a signal which, although very weak, can be detected and localized by copper coils placed around the patient. An image representing the distribution of the hydrogen protons can be built up (Fig. 1.14). The strength of the signal depends not only on proton density but also on two relaxation times, T1 and T2; T1 depends on the time the protons take to return to the axis of the magnetic field, and T2 depends on the time the protons take to dephase (also known as T2 decay). A T1-weighted image is one in which the contrast between tissues is due mainly to their T1 relaxation properties, while in a T2-weighted image the contrast is due to the T2 relaxation properties (Table 1.1). Some sequences produce images that approximate mainly to proton density. Most pathological processes show increased T1 and T2 relaxation times and, therefore, these processes appear lower in signal (black) on a T1-weighted scan and higher in signal intensity (whiter) on a T2-weighted image than the normal surrounding tissues. The T1- and T2-weighting of an image can be selected by appropriately altering the timing and sequence of radiofrequency pulses.

There are many other sequences with a bewildering variety of names and acronyms. They are designed to highlight different tissue characteristics, for example to demonstrate water content (HASTE sequence), diminish the signal from fat and so highlight pathology or contrast enhancement (fat suppression or STIR sequence, see Fig. 6.43), or demonstrate the combination of water and lipid content in

the same voxel (chemical shift imaging, see Fig. 10.17). Dynamic contrast-enhanced images (DCE-MRI) using gadolinium contrast medium (see below) may be used to demonstrate the anatomy of the large vessels as well as the enhancement characteristics of tumour angiogenesis (Fig. 1.14c). More recent developments include diffusion-weighted imaging and magnetic resonance spectroscopy, which can further characterize tissues and are often used in tumour assessment (Fig. 1.15).


A typical MRI scanner (Fig. 1.16) consists of a large circular magnet. Inside the magnet are the radiofrequency transmitter and receiver coils, as well as gradient coils to allow spatial localization of the MRI signal. Ancillary equipment converts the signals into a digital form, which the computer can manipulate to create an image. One advantage of MRI over CT is that the information can be directly imaged in any plane. In most instances, MRI requires a longer scan time (often several minutes) compared with CT, with the disadvantage that the patient has to keep still during the scanning procedure. Unavoidable movements from breathing, cardiac pulsation and peristalsis often degrade the image. Techniques to speed up scan times and limit the effect of motion by the use of various electronic methods have been introduced. Cardiac gating and breath-hold sequences are now readily available.

Magnetic resonance imaging gives very different information to CT. The earliest successful application was for scanning the brain and spinal cord, where MRI has significant advantages over CT and few disadvantages. MRI is now also an established technique for imaging the spine, bones, joints, pelvic organs, liver, biliary system, urinary tract and heart. At first sight it may seem rather surprising that MRI provides valuable information in skeletal disease as calcified tissues do not generate any signal during the procedure. This seeming paradox is explained by the fact that MRI provides images of the bone marrow and the soft tissues inside and surrounding joints (Fig. 1.17).


The physical basis of imaging blood vessels with MRI is complicated and beyond the scope of this book. Suffice it to say that, with some sequences, fast-flowing blood produces no signal (Fig. 1.18), whereas with others it produces a bright signal. This 'motion effect' can be exploited to image blood vessels. Such flow-sensitive sequences are mostly used for head and neck imaging, for example intracranial arteriovenous malformations and stenoses of the

Table 1.1 Appearance of water and fat on different magnetic resonance sequences


Sequence	Water signal intensity	Fat signal intensity
T1-weighted	Low	High
T2-weighted	High	High
T1 with fat saturation	Low	Low
T2 with fat saturation	High	Low

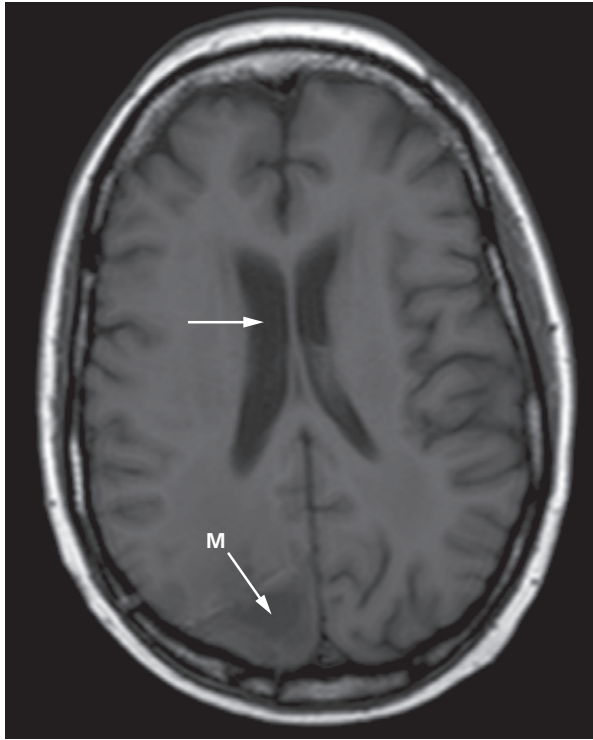

(a)

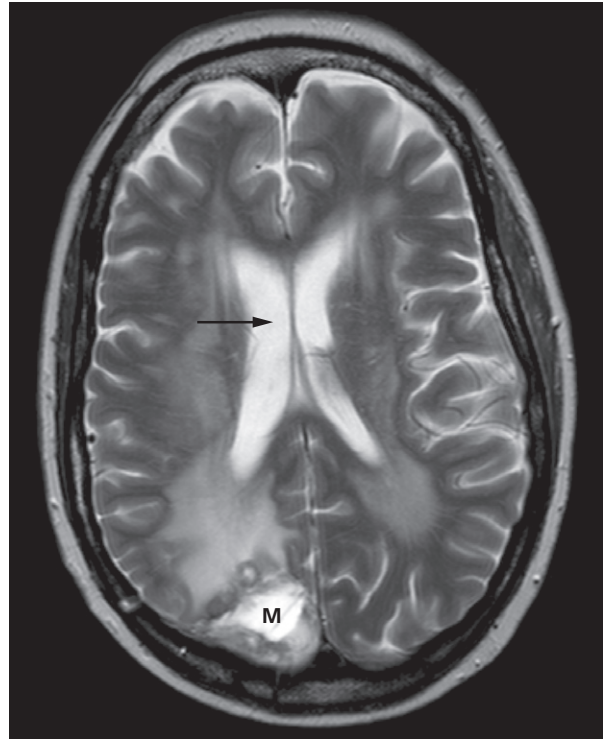

(b)

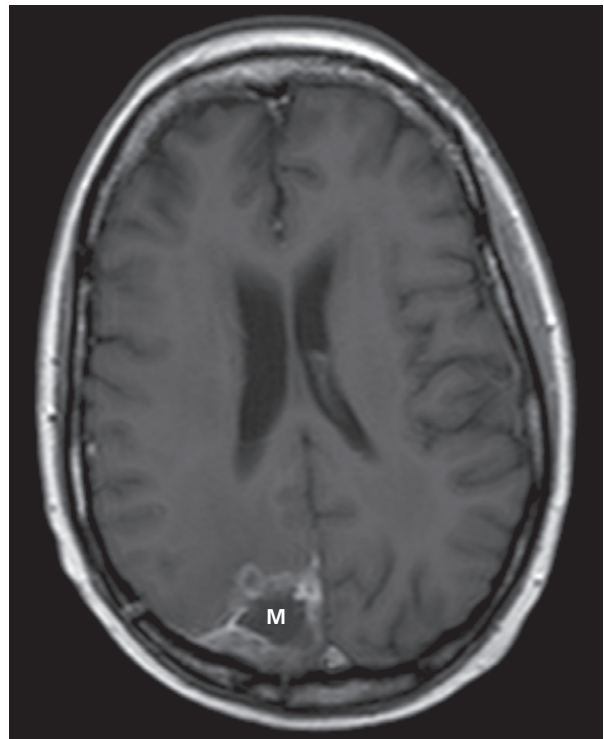

(c)


Fig. 1.14 MRI of brain. (a) Axial T1-weighted image. (b) Axial T2-weighted image. (c) Axial T1-weighted image following gadolinium. Note that the cerebrospinal fluid within the lateral ventricles is of low signal intensity on T1- and high signal intensity on T2-weighted images (arrows in (a) and (b)). Note also that the intensity of the white and grey matter of the brain differs on the two images. There is a metastasis from a breast carcinoma (M) in the right occipital pole, showing oedema around the mass on the T2-weighted image and enhancement on the post contrast image.

carotid arteries can be readily demonstrated without contrast media. The resulting images resemble a conventional angiogram (Fig. 1.19).


Magnetic resonance imaging of the heart uses electronic gating to obtain images during a specific portion of the cardiac cycle. With this technique it is possible to limit the degradation of the image by cardiac motion and demonstrate the cardiac chambers, valves and myocardium.

Alternatively, the beating heart can be directly visualized as a cine image.

One of the advantages of MRI is that it involves no ionizing radiation. The strong magnetic fields, however, mean that it is at present contraindicated in patients with certain implantable devices, including cardiac pacemakers, certain types of aneurysm clip and intraocular metallic foreign bodies.

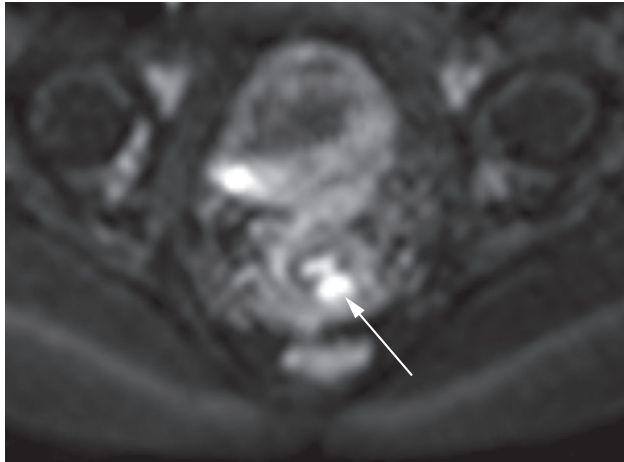


(a)

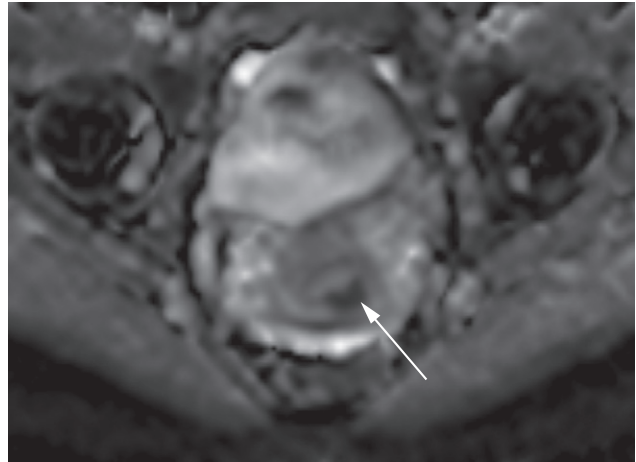

(b)

Fig. 1.15 Diffusion-weighted imaging. (a) A diffusion-weighted image with b value 750 demonstrating a small cervix cancer with high signal intensity (arrow). (b) The corresponding apparent diffusion coefficient (ADC) map demonstrates low signal intensity at the same position (arrow). This combination of high signal intensity on the high b value image and low signal intensity on the ADC map is consistent with restricted water diffusion, a characteristic feature of many cancers.

Fig. 1.16 Diagram of an MRI machine. The patient lies within a strong magnet (usually a cylindrical magnet). The radiofrequency transmitter coils send radiowaves into the patient and the same coils receive signals from within the patient. The intensity and source of these signals can be calculated and displayed as an image.

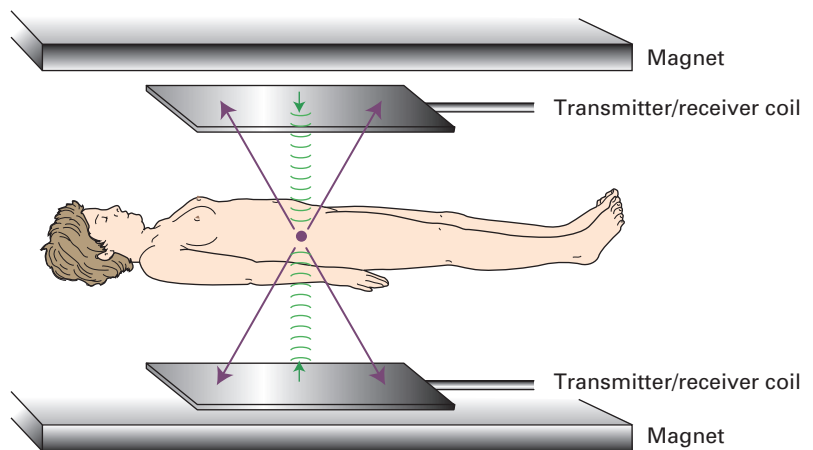

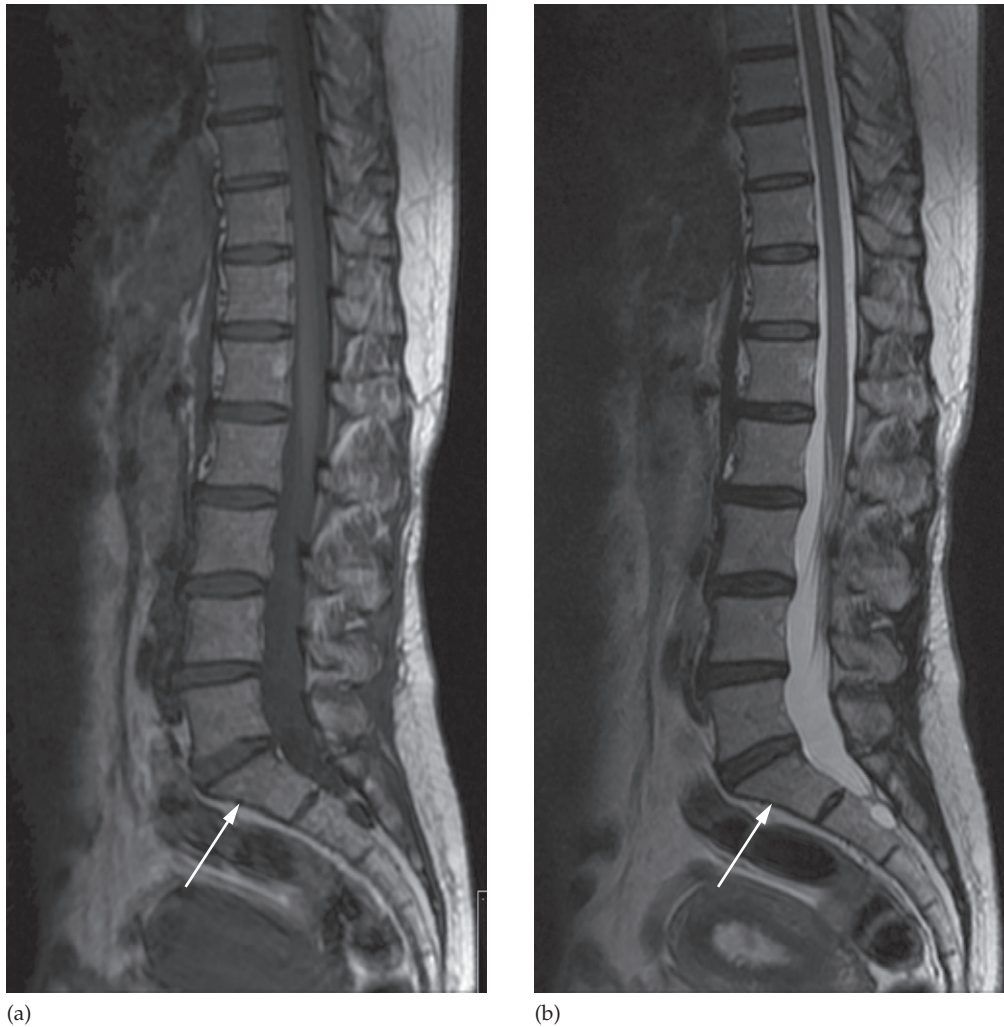


Fig. 1.17 MRI of a sagittal section of lumbar spine. (a) On this T1 sequence, the spinal cord is grey, cerebrospinal fluid (CSF) is nearly black and subcutaneous fat is white. (b) T2-weighted sequence. Here the CSF is white. Cortical bone (arrows) returns no signal and appears as a black line on both sequences. The fat in the bone marrow produces a signal that enables the vertebrae to be visualized.

Contrast agents for magnetic resonance imaging

Just as contrast media have been of great value in CT, magnetic contrast materials are providing useful diagnostic information with MRI. The most widely used agents are gadolinium compounds which only cross the blood–brain barrier when it is damaged by disease (see Fig. 1.14c), and which concentrate in tissues and disease processes with a

high blood supply. Tissues that concentrate the agent show very high signal intensity (i.e. they appear white) on T1-weighted images. Tissue-specific media, such as hepatocyte-specific agents and iron oxide agents for reticuloendothelial cell imaging, are also used. A particular application of contrast-enhanced MRI is magnetic resonance angiography, which along with CT angiography is gradually replacing conventional diagnostic angiography.